



**Title: Monitoring of Particulate Matter (PM) Emissions**

**Permit Number:** PPC/204  
**Operator:** Steel Construction Limited  
**Installation:** Spray Painting Area (LHS & RHS)  
**Monitoring Dates:** 13 September 2021

Reference Number: EI/8939

Client Organisation: Steel Construction Limited  
Address: Bodmin Road  
Coventry  
CV2 5DB

Monitoring Organisation: CES Environmental Instruments Ltd  
Address: Bretby Business Park  
Ashby Road  
Burton on Trent  
Staffordshire  
DE15 0YZ

Date of Report: 24 September 2021

Report Prepared By: Shane Elton  
MCERTS Registration Number: MM 04 532 (Level 2, TE1, TE2, TE3, TE4)

Signed:

Report Approved By: Robert Allen  
MCERTS Registration Number: MM 02 009 (Level 2, TE1, TE2, TE3, TE4)

Signed:

**Contents**

Part 1: Executive Summary .....3  
    1.1 Monitoring Objectives .....3  
    1.2 Monitoring Results .....4  
    1.3 Operating Information .....4  
    1.4 Monitoring Deviations.....5  
  
Part 2: Supporting Information.....6  
    Appendix 1 General Information.....6  
    Appendix 2 Diagrams of Emission Point .....8  
    Appendix 3 Particulate Matter (Sampling Measurement & Results) .....10  
    Appendix 4 Calibration Certificates .....21  
    Appendix 5 Uncertainty Calculations.....24

## **Part 1: Executive Summary**

### **1.1 Monitoring Objectives**

Steel Construction Limited placed a contract with CES Environmental Instruments Ltd for the compliance check monitoring of emissions to air from the Spray Painting Area (LHS & RHS).

#### **Spray Painting Area (LHS & RHS)**

Steel Construction Ltd operates a factory manufacturing steel parts for the construction industry at their Coventry site.

The metal products being sprayed arrive at the premises shot blasted and sometimes primed. The application of paints to steel beams, by airless spraying, occurs inside a wet wall spray booth. All emissions from the spray booth are released to atmosphere. The sludge from the wet filtration is removed and collected by a waste disposal company.

The test work was undertaken on 13 September 2021 by CES Environmental Instruments Ltd Engineers and carried out as part of CES Environmental Instruments Ltd job reference EI/8939.

The substances monitored were:-

Particulate Matter

On the day of testing there were no special requirements for the monitoring.

## 1.2 Monitoring Results

Emission Point Reference: Spray Painting Area (LHS)

Substance to be Monitored	Emission Limit Value	Periodic Monitoring Result	Uncertainty of Measurement (95% CI)	Blank Result	Units	Reference Conditions	Emission Rate	Date of Sampling	Start and End Times	Monitoring Method Reference	Accreditation for use of Method	Operating Status
Particulate Matter	50	0.11	0.63	0.05*	mg/m <sup>3</sup>	273K, 101.3kPa	0.001 kg/hr	13 September 2021	09:39-10:43	BS EN 13284-1	UKAS & MCERTS	Normal Operation

\* Indicates where a value less than the limit of detection of the weighing procedure (0.09mg) has been reported, the value lies between the detection limit and zero. A value of half the limit of detection (0.045mg) has been used to calculate the concentration.

Emission Point Reference: Spray Painting Area (RHS)

Substance to be Monitored	Emission Limit Value	Periodic Monitoring Result	Uncertainty of Measurement (95% CI)	Blank Result	Units	Reference Conditions	Emission Rate	Date of Sampling	Start and End Times	Monitoring Method Reference	Accreditation for use of Method	Operating Status
Particulate Matter	50	0.45	0.63	0.05*	mg/m <sup>3</sup>	273K, 101.3kPa	0.006 kg/hr	13 September 2021	10:55-11:59	BS EN 13284-1	UKAS & MCERTS	Normal Operation

\* Indicates where a value less than the limit of detection of the weighing procedure (0.09mg) has been reported, the value lies between the detection limit and zero. A value of half the limit of detection (0.045mg) has been used to calculate the concentration.

## 1.3 Operating Information

Emission Point Reference: Spray Painting Area (LHS)

Process Type	Batch Sample Details	Fuel	Product	Load	Abatement
Batch	Phosphate 14B420 – Grey Primer	-	Steel Parts	Beams	Bag Filter

Emission Point Reference: Spray Painting Area (RHS)

Process Type	Batch Sample Details	Fuel	Product	Load	Abatement
Batch	Phosphate 14B420 – Grey Primer	-	Steel Parts	Beams	Bag Filter

Comparison of Operator CEMS and Periodic Monitoring Results								
Substance to be Monitored	Emission Limit Value	Periodic Monitoring Result	Uncertainty of Measurement (95% CI)	Units	Reference Conditions	Date of Sampling	Start and End Times	CEMS Results
Particulate Matter (LHS)	50	0.11	0.63	mg/m <sup>3</sup>	273K, 101.3kPa	13 September 2021	09:39-10:43	No Data Available
Particulate Matter (RHS)	50	0.45	0.63	mg/m <sup>3</sup>	273K, 101.3kPa	13 September 2021	10:55-11:59	No Data Available

#### 1.4 Monitoring Deviations

The sample plane does not comply upstream and downstream as per the requirements of BS EN 15259.  
Only one sample port available.

## **Part 2: Supporting Information**

### **Appendix 1 General Information**

### CES Environmental Instruments Ltd staff details

Name	Role	MCERT Registration Number	Level 1	Level 2	TE1	TE2	TE3	TE4	At site
Shane Elton	Team Leader	MM 04 532		✓	✓	✓	✓	✓	T
				Mar 2023	Dec 2021	Dec 2024	Mar 2024	Mar 2023	
Stephen Cashmore	Technician	MM 18 1502	✓						✓
				Sept 2023					

T = Nominated Team Leader on Site

### CES Environmental Instruments Ltd method details

Pollutant	Method	CES Procedure
Particulate Matter	BS EN 13284-1	WI 4/1
Moisture	BS EN 14790	WI 4/40

### Monitoring Equipment Used

Gravimat & Probe

CES Environmental Instruments Ltd Reference: C231

## **Appendix 2**

### **Diagrams of Emission Point**





## Sampling Location

Dimensions	Cross Sectional Area	Orientation	Sample Ports Available/Used	Sampling Positions Per Plane	Standard
Dia =700mm	0.385m <sup>2</sup>	Vertical	1/1	3	BS EN 15259
<p><b>Comments:</b>  Sample ports: 1 off 4" BSP sockets bolted onto flanges</p> <p>Sample times are calculated from the total sample time equally divided by the no. of sample positions per plane. The minimum sample time per position is 3 minutes.</p> <p>Sample positions calculated using the General method for circular ducts</p> <p>Pitot Traverse  Along lines A &amp; B at positions consistent with BS EN 15259 these positions are:  11.3%, 50.0%, 88.7%</p> <p>Sample Positions  Along lines A &amp; B at as many of the positions required within the standard method as can be achieved given the clearance limitations behind each socket. BS EN 15259 requires sampling at 3 points (3 on one line) these positions are:  11.3%, 50.0%, 88.7%</p>					
				Yes	No
<b>Has homogeneity test been carried out?</b>					✓
<b>If Yes - Is stack gas homogenous?</b>					
<b>Any physical or regulatory restrictions regarding usage of equipment?</b> N/A					

Compliance with BS EN 15259 / EA TGN M1	Yes	No
<b>Does the sample plane comply upstream?</b>		✓
<b>Does the sample plane comply downstream?</b>		✓
<b>Are the appropriate sample ports fitted?</b>	✓	
<b>Do the stack gas velocity / temperature profiles comply?</b>	✓	
<b>Minimum platform area &gt;5m<sup>2</sup></b>	✓	



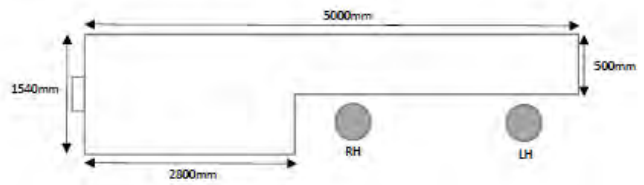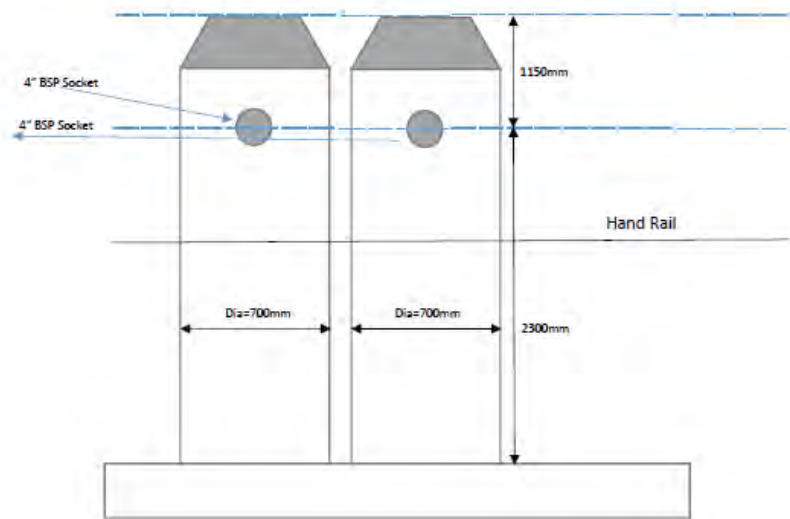

**Appendix 3**  
**Particulate Matter (Sampling Measurement & Results)**

**Site :** Steel Construction Limited  
**Date :** 13 September 2021  
**Plant :** Spray Painting Area (LHS)  
**File Ref.** 8939

**Mean Particulate Results**

Filter	Time	mg/m <sup>3</sup> (Actual Conditions)	m <sup>3</sup> /hr	mg/Nm <sup>3</sup> (Reference Conditions)	Nm <sup>3</sup> /hr	kg/hr
80663	09:39-10:10	0.10	13352	0.11	12604.0	0.001
80907	10:12-10:43	0.09	13398	0.10	12648.0	0.001
	<b>Mean</b>	<b>0.10</b>	<b>13375</b>	<b>0.11</b>	<b>12626.00</b>	<b>0.001</b>

**Control Blank Filter**

Filter	Volume (m <sup>3</sup> )	
80663	0.825	
80907	0.824	
<b>Mean</b>	<b>0.825</b>	(Reference Conditions with no correction for Oxygen)

**Filter** 522061

<b>Tare Weight</b>	17230.44 mg	
<b>Gross Weight</b>	17230.49 mg	*
<b>Gain</b>	0.04 mg	
<b>Measured Oxygen</b>	%	
<b>Concentration</b>	0.05 mg/Nm <sup>3</sup>	

Results Correct to

Temperature		Pressure		Oxygen		Gas	
°C/K	0/273	mbar/kPa	1013/101.3	%		Wet/Dry	Wet

\* Indicates where a value less than the limit of detection of the weighing procedure (0.09mg) has been reported, the value lies somewhere between the detection limit and zero. A value of half the limit of detection (0.045mg) has been used to calculate the concentration.

protocol simultaneous isokinetic extraction measurement

13/09/2021 09:39

13/09/2021 10:10

collector-no. 663  
 engineer SE,SC  
 plant name Spray Painting Area LHS  
 place Steel Construction  
 remarks Normal Operation  
 Diam:700mm  
 T1

operating parameter

normal density humid [ kg / m<sup>3</sup> ] : 1.25  
 water vapour [ %Vol ] : 3  
 ambient pressure [ mbar ] : 1011  
 duct cross-section [ m<sup>2</sup> ] : 0.385

extraction parameter

change of meas. point [h:m:s] : 00:10:00  
 points / axis : 3  
 nozzles diameter [ mm ] : 8  
 isokinetic factor : 1  
 tare weight [ mg ] : 17539.67  
 gross weight [ mg ] : 17539.76

evaluation

meas. time [h:m:s] : 00:30:00  
 dust weight [ mg ] : 0.09

extracted partial volume  
 actual conditions [ m<sup>3</sup> ] : 0.874  
 in norm wet [ Nm<sup>3</sup> ] : 0.825  
 in norm dry [ Nm<sup>3</sup> ] : 0.800

volume flow in duct  
 actual conditions [m<sup>3</sup>/h] : 13352  
 in norm wet [Nm<sup>3</sup>/h] : 12604  
 in norm dry [Nm<sup>3</sup>/h] : 12226

dust concentration  
 actual conditions [mg/m<sup>3</sup> ] : 0.10  
 in norm wet [mg/Nm<sup>3</sup> ] : 0.11  
 in norm dry [mg/Nm<sup>3</sup> ] : 0.11

protocol simultaneous isokinetic extraction measurement

13/09/2021 09:39

13/09/2021 10:10

measured values table

axis	depth	T_probe [°C]	v_duct [m/s]	angle [grd]	Q_act. [m³/h]	volume [m³]	meas. time [ H:M:S ]	p10 [mbar]	p40 [mbar]
1	1	17	9.6	0.8	1.76	0.293	00:10:00	2.00	-57
1	2	17	9.7	0.6	1.75	0.291	00:10:00	2.00	-57
1	3	17	9.6	0.5	1.74	0.290	00:10:00	2.00	-57
		17	9.6	0.6	1.75	0.291		2.00	-57

protocol simultaneous isokinetic extraction measurement

13/09/2021 10:12

13/09/2021 10:43

collector-no. 907  
 engineer SE,SC  
 plant name Spray Painting Area LHS  
 place Steel Construction  
 remarks Normal Operation  
 Diam:700mm  
 T2

operating parameter

normal density humid [ kg / m<sup>3</sup> ] : 1.25  
 water vapour [ %Vol ] : 3  
 ambient pressure [ mbar ] : 1011  
 duct cross-section [ m<sup>2</sup> ] : 0.385

extraction parameter

change of meas. point [h:m:s] : 00:10:00  
 points / axis : 3  
 nozzles diameter [ mm ] : 8  
 isokinetic factor : 1  
 tare weight [ mg ] : 17663.41  
 gross weight [ mg ] : 17663.49

evaluation

meas. time [h:m:s] : 00:30:00  
 dust weight [ mg ] : 0.08

extracted partial volume  
 actual conditions [ m<sup>3</sup> ] : 0.873  
 in norm wet [ Nm<sup>3</sup> ] : 0.824  
 in norm dry [ Nm<sup>3</sup> ] : 0.799

volume flow in duct  
 actual conditions [m<sup>3</sup>/h] : 13398  
 in norm wet [Nm<sup>3</sup>/h] : 12648  
 in norm dry [Nm<sup>3</sup>/h] : 12268

dust concentration  
 actual conditions [mg/m<sup>3</sup> ] : 0.09  
 in norm wet [mg/Nm<sup>3</sup> ] : 0.10  
 in norm dry [mg/Nm<sup>3</sup> ] : 0.10

protocol simultaneous isokinetic extraction measurement

13/09/2021 10:12

13/09/2021 10:43

measured values table

axis	depth	T_probe [°C]	v_duct [m/s]	angle [grd]	Q_act. [m³/h]	volume [m³]	meas. time [ H:M:S ]	p10 [mbar]	p40 [mbar]
1	1	17	9.7	0.0	1.74	0.291	00:10:00	2.00	-58
1	2	17	9.6	-0.1	1.74	0.290	00:10:00	2.00	-59
1	3	17	9.7	-0.1	1.75	0.292	00:10:00	2.00	-59
		17	9.7	-0.1	1.74	0.291		2.00	-59



**Site :** Steel Construction Limited  
**Date :** 13 September 2021  
**Plant :** Spray Painting Area (RHS)  
**File Ref.** 8939

**Mean Particulate Results**

Filter	Time	mg/m <sup>3</sup> (Actual Conditions)	m <sup>3</sup> /hr	mg/Nm <sup>3</sup> (Reference Conditions)	Nm <sup>3</sup> /hr	kg/hr
802157	10:55-11:26	0.35	13537	0.37	12779.0	0.005
802007	11:28-11:59	0.50	13398	0.53	12648.0	0.007
<b>Mean</b>		<b>0.43</b>	<b>13468</b>	<b>0.45</b>	<b>12713.50</b>	<b>0.006</b>

**Control Blank Filter**

Filter	Volume (m <sup>3</sup> )	
802157	0.834	
802007	0.826	
<b>Mean</b>	<b>0.830</b>	(Reference Conditions with no correction for Oxygen)

**Filter** 522057

<b>Tare Weight</b>	17282.16 mg	
<b>Gross Weight</b>	17282.21 mg	*
<b>Gain</b>	0.04 mg	
<b>Measured Oxygen</b>	%	
<b>Concentration</b>	0.05 mg/Nm <sup>3</sup>	

Results Correct to

Temperature		Pressure		Oxygen		Gas	
°C/K	0/273	mbar/kPa	1013/101.3	%		Wet/Dry	Wet

\* Indicates where a value less than the limit of detection of the weighing procedure (0.09mg) has been reported, the value lies somewhere between the detection limit and zero. A value of half the limit of detection (0.045mg) has been used to calculate the concentration.

protocol simultaneous isokinetic extraction measurement

collector-no. 2157  
 engineer SE,SC  
 plant name Spray Painting Area RHS  
 place Steel Construction  
 remarks Normal Operation  
 Diam:700mm  
 T1

operating parameter

normal density humid [ kg / m<sup>3</sup> ] : 1.25  
 water vapour [ %Vol ] : 3  
 ambient pressure [ mbar ] : 1011  
 duct cross-section [ m<sup>2</sup> ] : 0.385

extraction parameter

change of meas. point [h:m:s] : 00:10:00  
 points / axis : 3  
 nozzles diameter [ mm ] : 8  
 isokinetic factor : 1  
 tare weight [ mg ] : 18635.62  
 gross weight [ mg ] : 18635.93

evaluation

meas. time [h:m:s] : 00:30:00  
 dust weight [ mg ] : 0.31

extracted partial volume  
 actual conditions [ m<sup>3</sup> ] : 0.883  
 in norm wet [ Nm<sup>3</sup> ] : 0.834  
 in norm dry [ Nm<sup>3</sup> ] : 0.809

volume flow in duct  
 actual conditions [m<sup>3</sup>/h] : 13537  
 in norm wet [Nm<sup>3</sup>/h] : 12779  
 in norm dry [Nm<sup>3</sup>/h] : 12395

dust concentration  
 actual conditions [mg/m<sup>3</sup> ] : 0.35  
 in norm wet [mg/Nm<sup>3</sup> ] : 0.37  
 in norm dry [mg/Nm<sup>3</sup> ] : 0.38

protocol simultaneous isokinetic extraction measurement

13/09/2021 10:55

13/09/2021 11:26

measured values table

axis	depth	T_probe [°C]	v_duct [m/s]	angle [grd]	Q_act. [m³/h]	volume [m³]	meas. time [ H:M:S ]	p10 [mbar]	p40 [mbar]
1	1	17	9.7	0.5	1.76	0.294	00:10:00	2.00	-52
1	2	17	9.8	0.5	1.77	0.295	00:10:00	2.00	-52
1	3	17	9.8	0.3	1.77	0.294	00:10:00	2.00	-52
		17	9.8	0.4	1.77	0.294		2.00	-52

protocol simultaneous isokinetic extraction measurement

13/09/2021 11:28

13/09/2021 11:59

collector-no. 2007  
 engineer SE,SC  
 plant name Spray Painting Area RHS  
 place Steel Construction  
 remarks Normal Operation  
 Diam:700mm  
 T2

operating parameter

normal density humid [ kg / m<sup>3</sup> ] : 1.25  
 water vapour [ %Vol ] : 3  
 ambient pressure [ mbar ] : 1011  
 duct cross-section [ m<sup>2</sup> ] : 0.385

extraction parameter

change of meas. point [h:m:s] : 00:10:00  
 points / axis : 3  
 nozzles diameter [ mm ] : 8  
 isokinetic factor : 1  
 tare weight [ mg ] : 18540.4  
 gross weight [ mg ] : 18540.84

evaluation

meas. time [h:m:s] : 00:30:00  
 dust weight [ mg ] : 0.44

extracted partial volume  
 actual conditions [ m<sup>3</sup> ] : 0.875  
 in norm wet [ Nm<sup>3</sup> ] : 0.826  
 in norm dry [ Nm<sup>3</sup> ] : 0.801

volume flow in duct  
 actual conditions [m<sup>3</sup>/h ] : 13398  
 in norm wet [Nm<sup>3</sup>/h] : 12648  
 in norm dry [Nm<sup>3</sup>/h] : 12268

dust concentration  
 actual conditions [mg/m<sup>3</sup> ] : 0.50  
 in norm wet [mg/Nm<sup>3</sup> ] : 0.53  
 in norm dry [mg/Nm<sup>3</sup> ] : 0.55

protocol simultaneous isokinetic extraction measurement

13/09/2021 11:28

13/09/2021 11:59

measured values table

axis	depth	T_probe [°C]	v_duct [m/s]	angle [grd]	Q_act. [m³/h]	volume [m³]	meas. time [ H:M:S ]	p10 [mbar]	p40 [mbar]
1	1	17	9.7	-1.5	1.75	0.292	00:10:00	2.00	-58
1	2	17	9.6	-0.7	1.74	0.290	00:10:00	2.00	-58
1	3	17	9.7	0.8	1.76	0.293	00:10:00	2.00	-59
		17	9.7	-0.5	1.75	0.292		2.00	-58

## **Appendix 4 Calibration Certificates**

## Certificate of Calibration

Date of Issue: 21st December 2020

Certificate No. CES1986  
Page 1 of 2

CES Environmental Instruments Ltd  
Bretby Business Park, Ashby Road  
Burton-on-Trent, Staffordshire, DE15 0YZ  
Tel: 01283 216334 Fax: 01283 550939

Certified By

### Instrument Details

Instrument Type	Gravimat SHC-502
Instrument Make	Erwin Sick
Instrument Serial No.	8118714
Quality No.	C231
Calibration Date	21/12/20
Calibrated By Name	S.Cashmore

### Ambient Conditions

Air Temperature (°C)	19
Barometric Pressure (mbar)	986
Relative Humidity (%)	60

### Instruments used to undertake calibration

E Type Pitot	UKAS Certificate No. K45800V	(Qu. No. C136)
Manometer Type FC012	UKAS Certificate No. 20002	(Qu. No. C082)
Manometer Type FC012	UKAS Certificate No. 20001	(Qu. No. C081)
Barometer Type 104	UKAS Certificate No. U103120-20	(Qu. No. C136)
Gallus Dry Gas Meter	UKAS Certificate No. N028407	(Qu. No. C333)
RIS Supercal XT	UKAS Certificate No. 3228080001	(Qu. No. C014)

### Flow and Extraction

The reference pitot was placed in a wind tunnel located at Bretby Business Park. The Gravimat SHC-5 Sampling Probe under test was mounted within the same wind tunnel in close proximity to the reference pitot. The wind tunnel was operated to generate a differential pressure across each pitot, a direct comparison was made. The differential pressures measured were in the region of the calibration points of the reference pitot. Correction factors were applied to the reference pitot and compared to the differential pressure shown for the pitot under test. The extraction system of the unit was operated for a period of one minute.

### Volume Flow

A calibrated dry gas meter was connected to the sampling nozzle of the Gravimat SCH-5. A volume of air is pulled through the sampling system. The measured value shown on the calibrated dry gas meter is then compared to the indicated value on the Gravimat SCH-5 display.

### Barometric Pressure

The barometric pressure was measured using a calibrated barometer. The indicated pressure was compared to the Gravimat SHC-5 display.

### Temperature

The probe thermocouple was placed in a thermocouple oven and heated. The temperature was measured using a calibrated thermocouple and temperature indicator. The resultant temperature was compared to the Gravimat SCH-5 display.

### Current

A mA current source was injected into the Gravimat SCH-5 using a mA current generator. The injected current was compared to the Gravimat SCH-5 display.

## Certificate of Calibration

Date of Issue: 21st December 2020

Certificate No. CES1986  
page 2 of 2

CES Environmental Instruments Ltd  
Bretby Business Park, Ashby Road  
Burton-on-Trent, Staffordshire, DE15 0YZ  
Tel: 01283 216334 Fax: 01283 550939

Certified By

### Instrument Details

Instrument Type Gravimat SHC-502  
Instrument Make Erwin Sick  
Instrument Serial No. 6118714  
Quality No. C231  
Calibration Date 21/12/20

### Ambient Conditions

Air Temperature (°C) 19  
Barometric Pressure (mbar) 986  
Relative Humidity (%) 60  
Air Density @ 0°C (kg/m³) 1.277  
Corrected Air Density (kg/m³) 1.1638

### Calibration Details

#### Flow and Extraction

	Pitot Correction	Applied Pressure Corrected (Pa)	SHC502 (Calculated) (Pa)	Pressure Factor	Calculated Velocity (m/s)	SHC502 Velocity (m/s)	Velocity Factor
5.4	0.988	5.3	5.2	1.02	3.028	3.000	1.01
40.6	0.988	40.1	39.1	1.03	8.303	8.200	1.01
86.5	0.990	85.6	83.8	1.02	12.131	12.000	1.01
171.1	0.990	169.4	166.2	1.02	17.061	16.900	1.01
231.6	0.988	228.8	223.5	1.02	19.830	19.600	1.01
<b>Mean (excluding 4.0Pa)</b>				<b>1.02</b>			<b>1.01</b>

#### Volume Flow

Nominal Flow Rate	Actual Flow Rate	Actual Flow Rate	Orifice Constant
l/min	l/min	m³/hr	
10.0	9.855	0.591	12.706
15.0	14.979	0.899	12.810
20.0	19.947	1.197	12.826
25.0	24.380	1.463	12.828
30.0	30.148	1.809	12.870
<b>Mean Orifice Constant (@1.5m³/hr) =</b>			<b>12.828</b>

#### Barometric Pressure

Pressure Input	
Required Value (mbar)	Indicated Value (mbar)
995.0	995.0
1001.0	1001.0
1014.0	1014.0

#### Temperature

Temperature Input	
Required Value (°C)	Indicated Value (°C)
25.0	25.1
50.0	50.1
100.0	99.8
150.0	150.2
250.0	250.4
300.0	300.0

#### Current

Current Value	
Required Value (mA)	Indicated Value (mA)
0	0.0
5	5.0
10	10.0
15	15.0
20	20.0

#### Time

Time Period mins	Required Value mins	Within Limit
3:00	2:59 → 3:01	Yes
5:00	4:59 → 5:01	Yes
10:00	9:59 → 10:01	Yes



## **Appendix 5 Uncertainty Calculations**

Uncertainty calculation for EN 13284 Determination of low range mass concentration of dust, Manual Gravimetric Method

Measurement Equation

$$c = \frac{m}{V} f_c$$

Limit value (ELV)	50 mg.m <sup>-3</sup>	Reference oxygen	% by volume
Measured concentration	0.11 mg.m <sup>-3</sup> (at reference conditions)		

Measured Quantities	Symbol	Value	Standard uncertainty	Units	Uncertainty as percentage	Uncertainty at lv	Requirement of std
Sampled Volume	V <sub>m</sub>	0.825	uV <sub>m</sub>	0.001 m <sup>3</sup>	0.12		<=2%
Sampled gas Temperature	T <sub>m</sub>	273	uT <sub>m</sub>	2 k	0.73		<=1%
Sampled gas Pressure	ρ <sub>m</sub>	101.3	uρ <sub>m</sub>	0.1 kPa	0.10		<=1%
Sampled gas Humidity	H <sub>m</sub>	0	uH <sub>m</sub>	1 % by volume	1.00		<=1%
Oxygen content	O <sub>2,m</sub>		uO <sub>2,m</sub>	0.1 % by volume	#DIV/0!		<=5%
Mass particulate	m	0.09	um	0.26 mg	288.89	0.63	<5% of limit value
Note - Sampled gas humidity, temperature and pressure are values at the gas meter							
Leak	L	2		%	2.00		<=2%
Uncollected Mass (Instack filter - no rinse)	UCM	0.009		mg	10		<=10%

Intermediate calculations				
Factor for std conds	fs	1.00		
uncertainty components	symbol	sensitivity coeff	u (in units of fs)	
	ρ <sub>m</sub>	0.010	0.001	
	H <sub>m</sub>	0.010	0.010	$f_s = \frac{(100 - H_m) 273 \rho_m}{100 T_m 101.3}$
	T <sub>m</sub>	0.004	0.007	
	ufs		0.012	1.24
Corrected volume	V	0.83	uV	0.010 m <sup>3</sup>
				1.25
Factor for O2 correction	fc	1.00		
uncertainty components	symbol	sensitivity coeff	u	
	O <sub>2,m</sub>	0.05	0.005	$f_c = \frac{21 - O_{2,ref}}{21 - O_{2,m}}$
Factor for O2 Correction	ufc	1.00		0.48

Parameter	Value	Units	Sensitivity coeff	Uncertainty contribution	Uncertainty as %
Corrected Volume (standard cc	V	0.83 m <sup>3</sup>	0.13	0.00 mg.m <sup>-3</sup>	1.25 %
Mass	m	0.09 mg	1.21	0.32 mg.m <sup>-3</sup>	288.89 %
Factor for O2 Correction	fc	1.00	0.11	0.00 mg.m <sup>-3</sup>	0.48 %
Leak	L	0.00 mg.m <sup>-3</sup>	1.00	0.00 mg.m <sup>-3</sup>	1.15 %
Uncollected mass	UCM	0.01 mg	1.21	0.01 mg.m <sup>-3</sup>	5.77 %
<b>Combined measurement uncertainty</b>				<b>0.32 mg.m<sup>-3</sup></b>	
Expanded uncertainty as percentage of measured value		577.90	% measured of value	expressed with a level of confidence of 95% (Using a coverage factor k=2)	
Expanded uncertainty in units of measurement		0.63	mg.m <sup>-3</sup>		
Expanded uncertainty as percentage of limit value		1.26	% ELV		

Verified

Uncertainty calculation for EN 13284 Determination of low range mass concentration of dust, Manual Gravimetric Method

Measurement Equation

$$c = \frac{m}{V} f_c$$

Limit value (ELV)	50 mg.m <sup>-3</sup>	Reference oxygen	% by volume
Measured concentration	0.53 mg.m <sup>-3</sup> (at reference conditions)		

Measured Quantities	Symbol	Value	Standard uncertainty	Units	Uncertainty as percentage	Uncertainty at lv	Requirement of std
Sampled Volume	V <sub>m</sub>	0.826	uV <sub>m</sub>	0.001 m <sup>3</sup>	0.12		<=2%
Sampled gas Temperature	T <sub>m</sub>	273	uT <sub>m</sub>	2 k	0.73		<=1%
Sampled gas Pressure	ρ <sub>m</sub>	101.3	uρ <sub>m</sub>	0.1 kPa	0.10		<=1%
Sampled gas Humidity	H <sub>m</sub>	0	uH <sub>m</sub>	1 % by volume	1.00		<=1%
Oxygen content	O <sub>2,m</sub>		uO <sub>2,m</sub>	0.1 % by volume	#DIV/0!		<=5%
Mass particulate	m	0.44	um	0.26 mg	59.09	0.63	<5% of limit value
Note - Sampled gas humidity, temperature and pressure are values at the gas meter							
Leak	L	2		%	2.00		<=2%
Uncollected Mass (Instack filter - no rinse)	UCM	0.044		mg	10		<=10%

Intermediate calculations				
Factor for std conds	fs	1.00		
uncertainty components	symbol	sensitivity coeff	u (in units of fs)	
	ρ <sub>m</sub>	0.010	0.001	
	H <sub>m</sub>	0.010	0.010	$f_s = \frac{(100 - H_m) 273 \rho_m}{100 T_m 101.3}$
	T <sub>m</sub>	0.004	0.007	
	ufs		0.012	1.24
Corrected volume	V	0.83	uV	0.010 m <sup>3</sup>
				1.25
Factor for O2 correction	fc	1.00		
uncertainty components	symbol	sensitivity coeff	u	
	O <sub>2,m</sub>	0.05	0.005	$f_c = \frac{21 - O_{2,ref}}{21 - O_{2,m}}$
Factor for O2 Correction	ufc	1.00	0.005	0.48

Parameter	Value	Units	Sensitivity coeff	Uncertainty contribution	Uncertainty as %
Corrected Volume (standard cc)	V	0.83 m <sup>3</sup>	0.64	0.01 mg.m <sup>-3</sup>	1.25 %
Mass	m	0.44 mg	1.21	0.31 mg.m <sup>-3</sup>	59.09 %
Factor for O2 Correction	fc	1.00	0.53	0.00 mg.m <sup>-3</sup>	0.48 %
Leak	L	0.01 mg.m <sup>-3</sup>	1.00	0.01 mg.m <sup>-3</sup>	1.15 %
Uncollected mass	UCM	0.03 mg	1.21	0.03 mg.m <sup>-3</sup>	5.77 %
<b>Combined measurement uncertainty</b>				<b>0.32 mg.m<sup>-3</sup></b>	
Expanded uncertainty as percentage of measured value		118.80	% measured of value	expressed with a level of confidence of 95% (Using a coverage factor k=2)	
Expanded uncertainty in units of measurement		0.63	mg.m <sup>-3</sup>		
Expanded uncertainty as percentage of limit value		1.27	% ELV		

Verified